


## INVERTED FLUORESCENCE MICROSCOPE

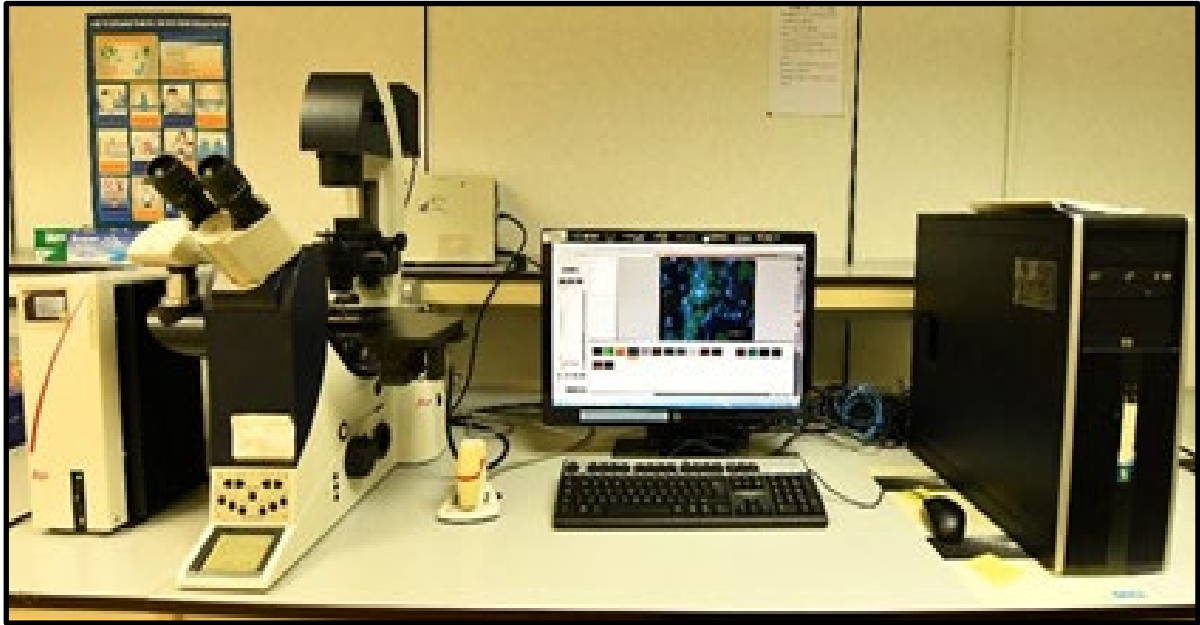

**Brand :** Leica

**Model :** DMI600B

**Brief description :**

- i) Connected to computer with software
- ii) Fluorescence use

**Sample requirement :** Observing cell and organisms in culture flask, microplate, roller bottles, microplates and petri dishes

**Limitation :** Not suitable for glass slide sample

**Location :** Cell Culture Room, Ground Floor, J16, Institute of Biological Sciences

**Person-in-charge :**

Assistant Science Officer :

1. Mohamad Fakhru Hisham bin Hashim  
Phone no. : +603-7967 6746  
Email : [syamyeeo@um.edu.my](mailto:syamyeeo@um.edu.my)

Science Officer :

1. Rozana binti Mohd Shah  
Phone no. : +603-7967 4389  
Email : [rozana@um.edu.my](mailto:rozana@um.edu.my)

**Service Charge details :**

ISB's User: RM20/3hour session

Collaborators: RM30/3hour session

UM's User: RM40/3hour session

Outside UM's User: RM70/3hour session

**STATUS**